


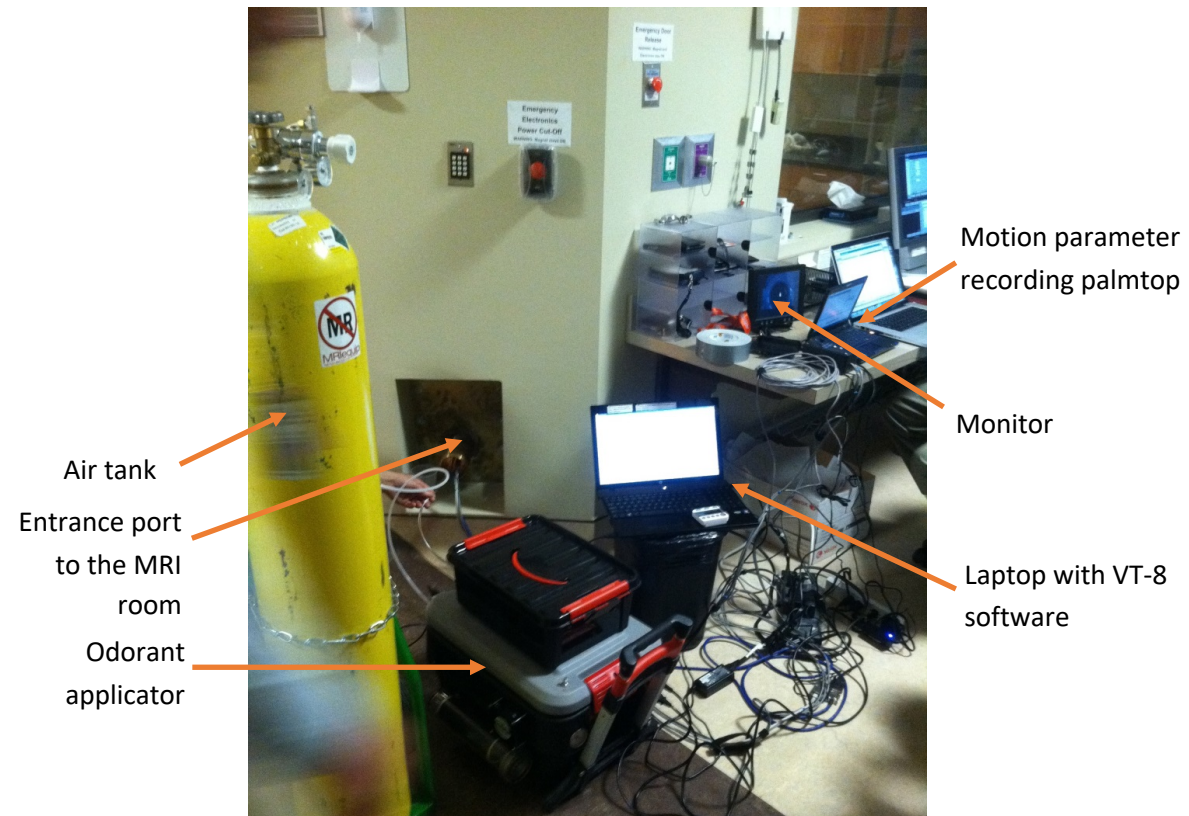

Air tank
Entrance port
to the MRI
room
Odorant
applicator

Motion parameter
recording palmtop
Monitor
Laptop with VT-8
software