

Figure 2

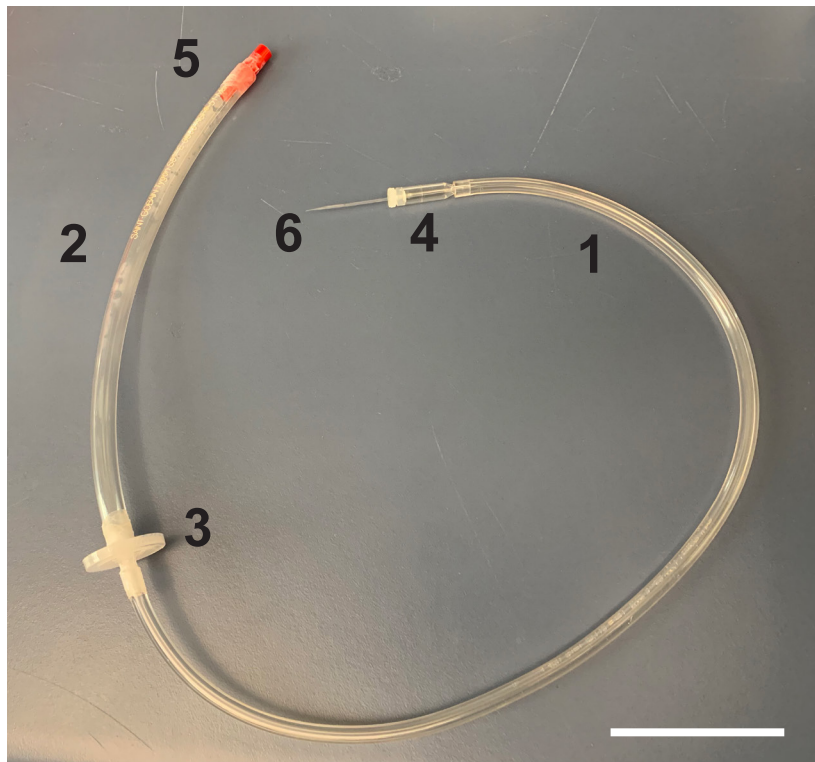


Figure 2. Assembly of mouth pipette

Mouth pipette is assembled by connecting narrow (1) and wide (2) tygon tubes with a PTFE filter (3). At the end of the narrow and wide tygon tube, capillary holder (4) and mouth piece (5) were attached, respectively. A hand-drawn glass capillary (6) can be inserted in the capillary holder. Scale bar is 50 mm.