

Figure 5

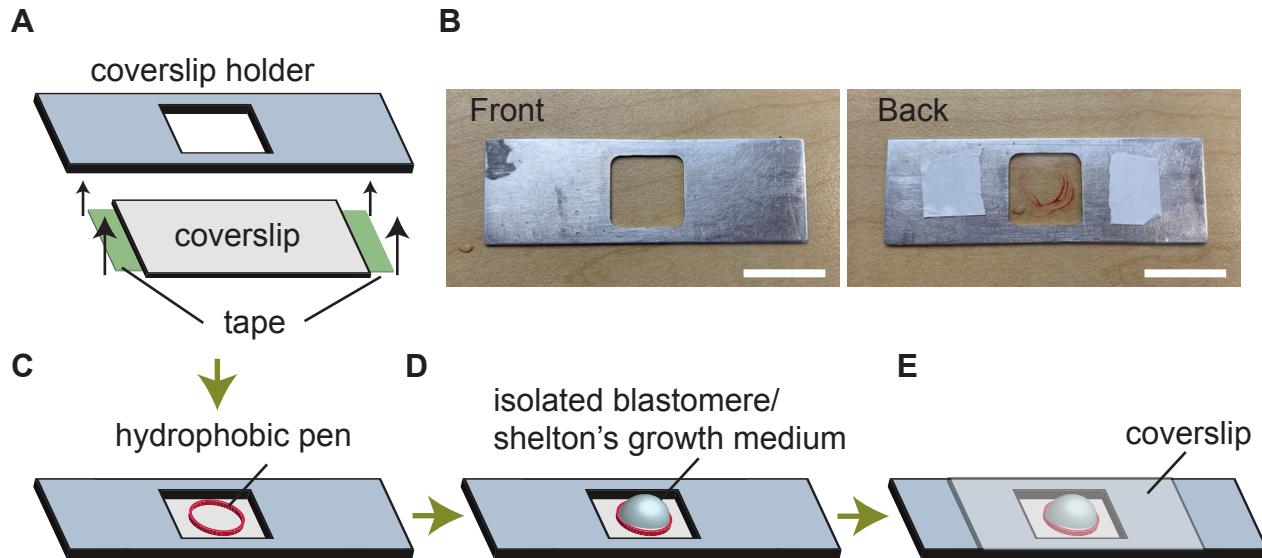


Figure 5. Assembly of imaging chamber

(A) Attaching coverslip to the coverslip holder. (B) Images of a coverslip holder. Coverslip holder before and after assembly is indicated on the left and right, respectively. (C) A circle drawn via a hydrophobic pen. (D) Addition of Shelton's growth medium and sample within the circle. (E) Mounting a coverslip to avoid evaporation. Scale bars show 50 mm.