
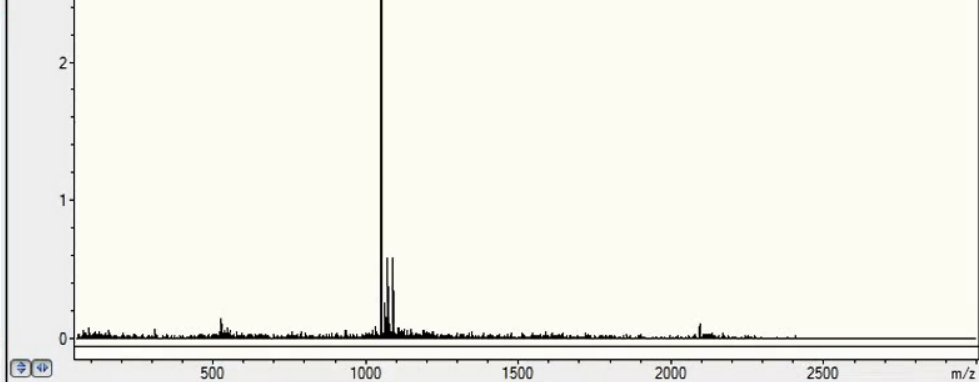
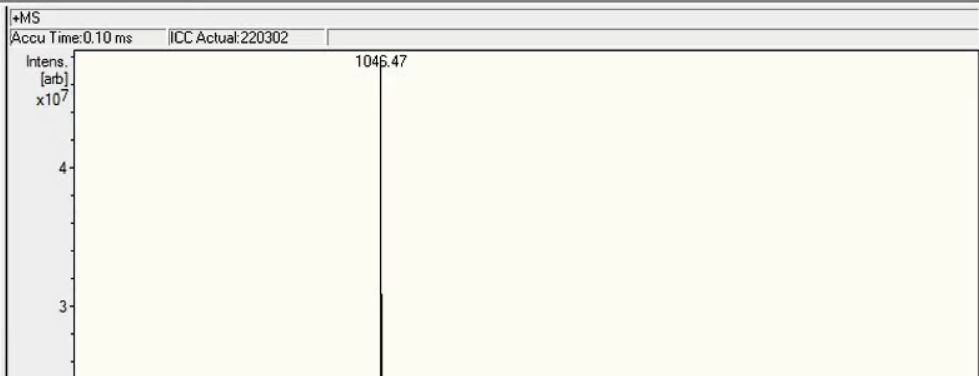
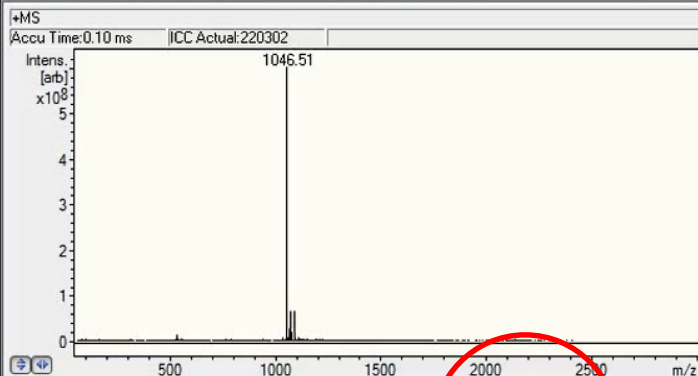




No connection

MS/MS

Last Run

5.01

View

Operate

Standby

Shutdown

☒ HV

- ☐ Auto MS(n)
- ☒ Manual MS(n)
- ☐ SmartMRM
- ☐ MRM

MS only

Mode Source Tune Manual MS(n) Sample Info Chromatogram Calibration

Data File

☒ Prefix/Counter ☐ Manual

Prefix AngiotensinII_ReferenceSample Counter 01

Subdirectory Default\JoVE

Path D:\data

Sample Parameter

Sample Name Dummy

Comment

Polarity

- ☒ Positive
- ☐ Negative
- ☐ Alternating

Edit Parameter

- ☒ Link Edit
- ☐ Unlink Edit for Parameter

☐ Apply to all Segments

Trap

Enhanced Resolution

☐ ICC Target 200000

Accu Time 0.10 ms

Scan 50 to 3000 m/z

Averages 10

Rolling Averaging

☐ On No. 1

Apply



user

Time Segm. # 1 MS

Changed Fore 1.31e-01 mbar High 3.89e-06 mbar