


A

Intra-run assay variation

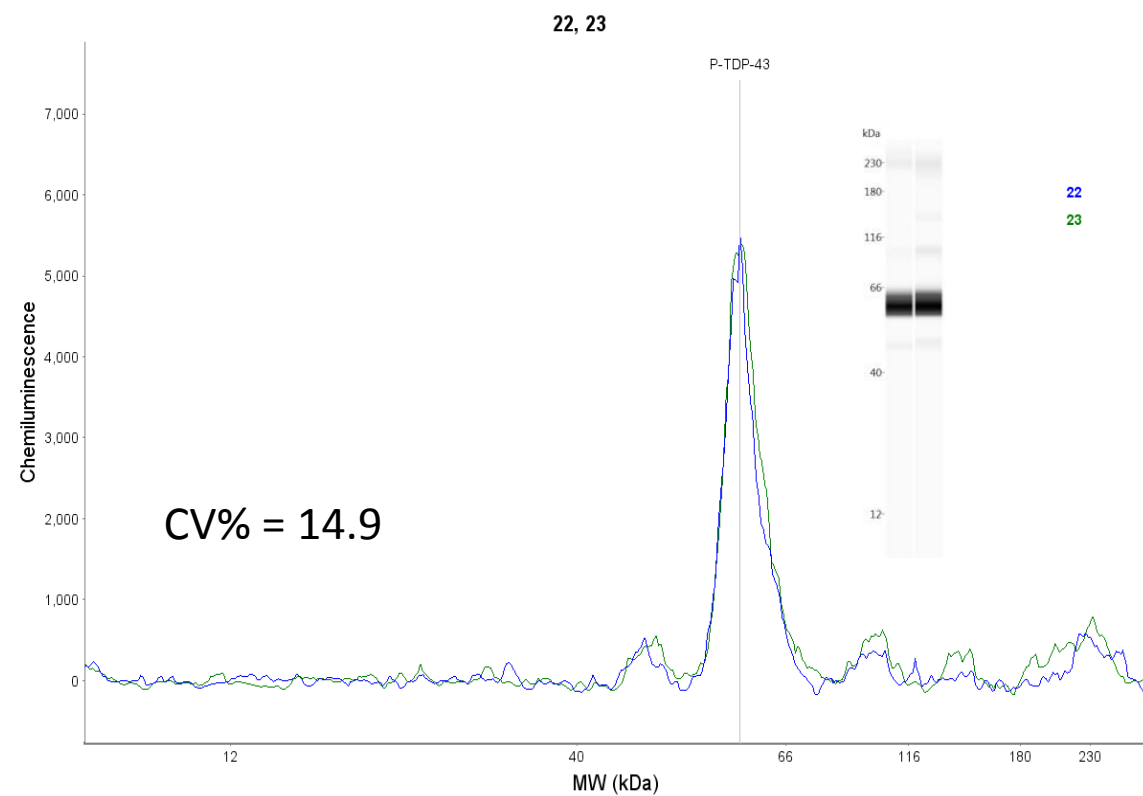

B

Inter-run assay variation

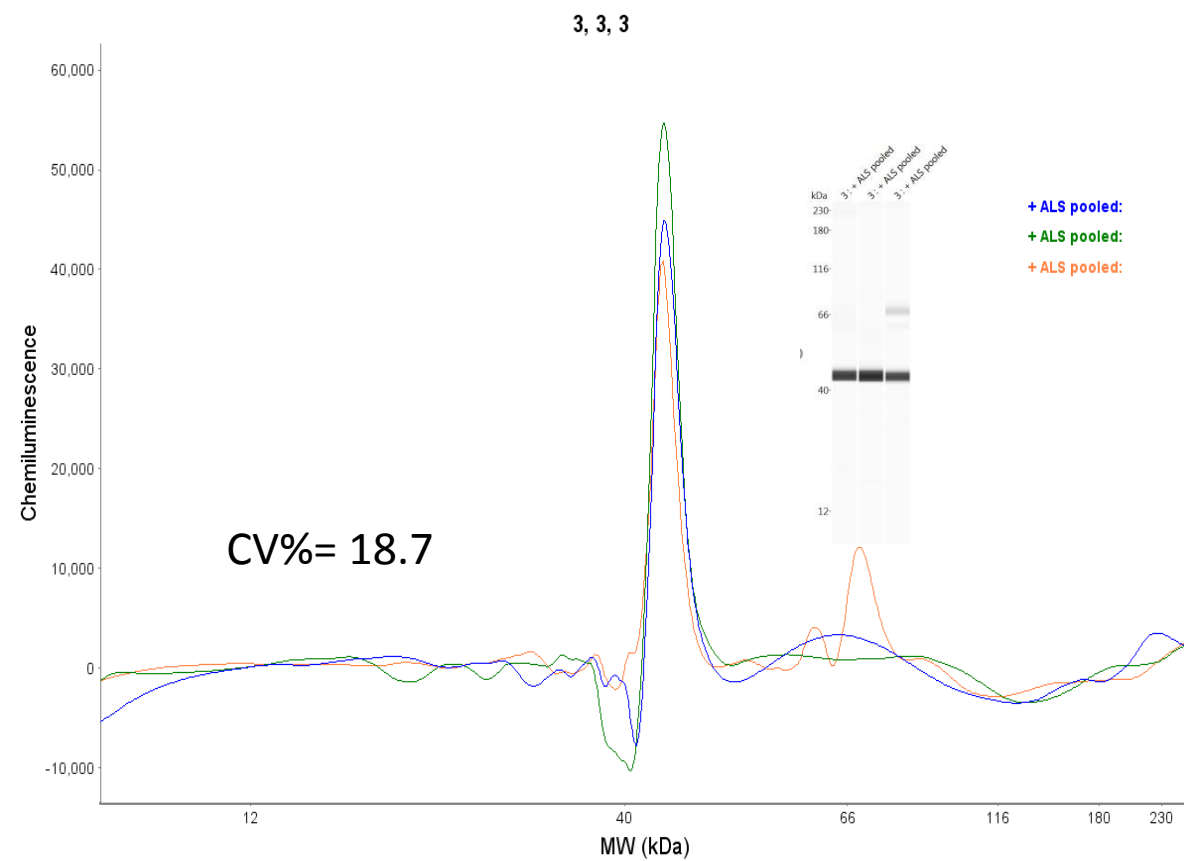


Fig.7