

Molecular Detection Software

Run Report

Run ID	MPN - Example	Run Date	8/4/2024 11:10:15 AM
Run Status	Completed	User	Joseph Capobianco
Technician	Joseph Capobianco	Report By	Joseph Capobianco
Run Comment	MPN - Example	Instrument	0218040024:218040024

	1	2	3	4	5	6	7	8	9	10	11	12
A												
B												
C												
D												
E												
F												
G												
H												

Well ID	Sample ID	Assay Type	Well Type	Kit Lot Number	Result	Comment
A1	10^0	Salmonella-2	Sample	8883705	Positive	
B1	10^0	Salmonella-2	Sample	8883705	Positive	
C1	10^0	Salmonella-2	Sample	8883705	Positive	
D1	10^0	Salmonella-2	Sample	8883705	Positive	
E1	10^0	Salmonella-2	Sample	8883705	Positive	
F1	10^0	Salmonella-2	Sample	8883705	Positive	
G1	10^0	Salmonella-2	Sample	8883705	Positive	
H1	10^0	Salmonella-2	Sample	8883705	Positive	
A2	10^-1	Salmonella-2	Sample	8883705	Positive	
B2	10^-1	Salmonella-2	Sample	8883705	Positive	
C2	10^-1	Salmonella-2	Sample	8883705	Positive	
D2	10^-1	Salmonella-2	Sample	8883705	Positive	

Molecular Detection Software

Run Report

Run ID	MPN - Example	Run Date	8/4/2024 11:10:15 AM
Run Status	Completed	User	Joseph Capobianco
Technician	Joseph Capobianco	Report By	Joseph Capobianco
Run Comment	MPN - Example	Instrument	0218040024:218040024

E2	10^-1	Salmonella-2	Sample	8883705	Positive	
F2	10^-1	Salmonella-2	Sample	8883705	Positive	
G2	10^-1	Salmonella-2	Sample	8883705	Positive	
H2	10^-1	Salmonella-2	Sample	8883705	Positive	
A3	10^-2	Salmonella-2	Sample	8883705	Positive	
B3	10^-2	Salmonella-2	Sample	8883705	Positive	
C3	10^-2	Salmonella-2	Sample	8883705	Positive	
D3	10^-2	Salmonella-2	Sample	8883705	Positive	
E3	10^-2	Salmonella-2	Sample	8883705	Positive	
F3	10^-2	Salmonella-2	Sample	8883705	Positive	
G3	10^-2	Salmonella-2	Sample	8883705	Positive	
H3	10^-2	Salmonella-2	Sample	8883705	Positive	
A4	10^-3	Salmonella-2	Sample	8883705	Positive	
B4	10^-3	Salmonella-2	Sample	8883705	Positive	
C4	10^-3	Salmonella-2	Sample	8883705	Positive	
D4	10^-3	Salmonella-2	Sample	8883705	Positive	
E4	10^-3	Salmonella-2	Sample	8883705	Positive	
F4	10^-3	Salmonella-2	Sample	8883705	Positive	
G4	10^-3	Salmonella-2	Sample	8883705	Positive	
H4	10^-3	Salmonella-2	Sample	8883705	Positive	
A5	10^-4	Salmonella-2	Sample	8883705	Positive	
B5	10^-4	Salmonella-2	Sample	8883705	Negative	
C5	10^-4	Salmonella-2	Sample	8883705	Positive	
D5	10^-4	Salmonella-2	Sample	8883705	Positive	
E5	10^-4	Salmonella-2	Sample	8883705	Positive	
F5	10^-4	Salmonella-2	Sample	8883705	Positive	
G5	10^-4	Salmonella-2	Sample	8883705	Negative	
H5	10^-4	Salmonella-2	Sample	8883705	Positive	
A6	10^-5	Salmonella-2	Sample	8883705	Negative	
B6	10^-5	Salmonella-2	Sample	8883705	Negative	




Molecular Detection Software

Run Report

Run ID	MPN - Example	Run Date	8/4/2024 11:10:15 AM
Run Status	Completed	User	Joseph Capobianco
Technician	Joseph Capobianco	Report By	Joseph Capobianco
Run Comment	MPN - Example	Instrument	0218040024:218040024

C6	10 ⁻⁵	Salmonella-2	Sample	8883705	Negative	
D6	10 ⁻⁵	Salmonella-2	Sample	8883705	Negative	
E6	10 ⁻⁵	Salmonella-2	Sample	8883705	Negative	
F6	10 ⁻⁵	Salmonella-2	Sample	8883705	Negative	
G6	10 ⁻⁵	Salmonella-2	Sample	8883705	Negative	
H6	10 ⁻⁵	Salmonella-2	Sample	8883705	Negative	









All Results

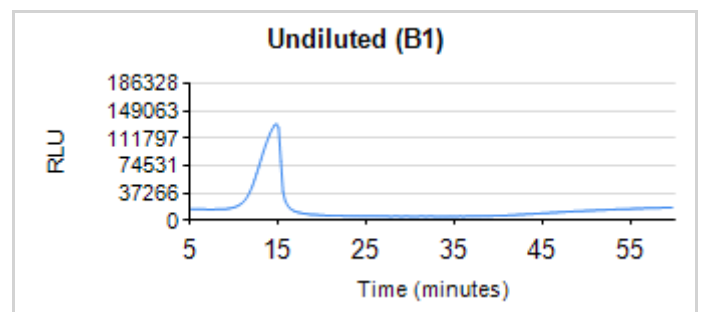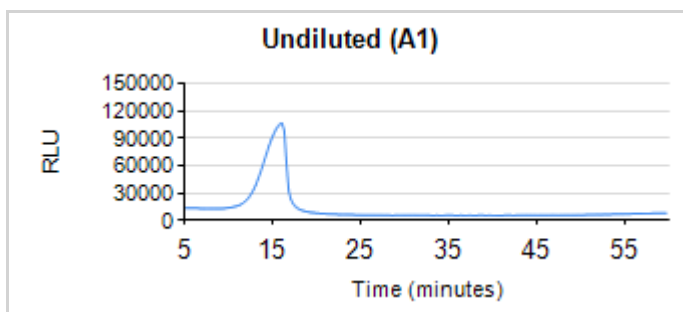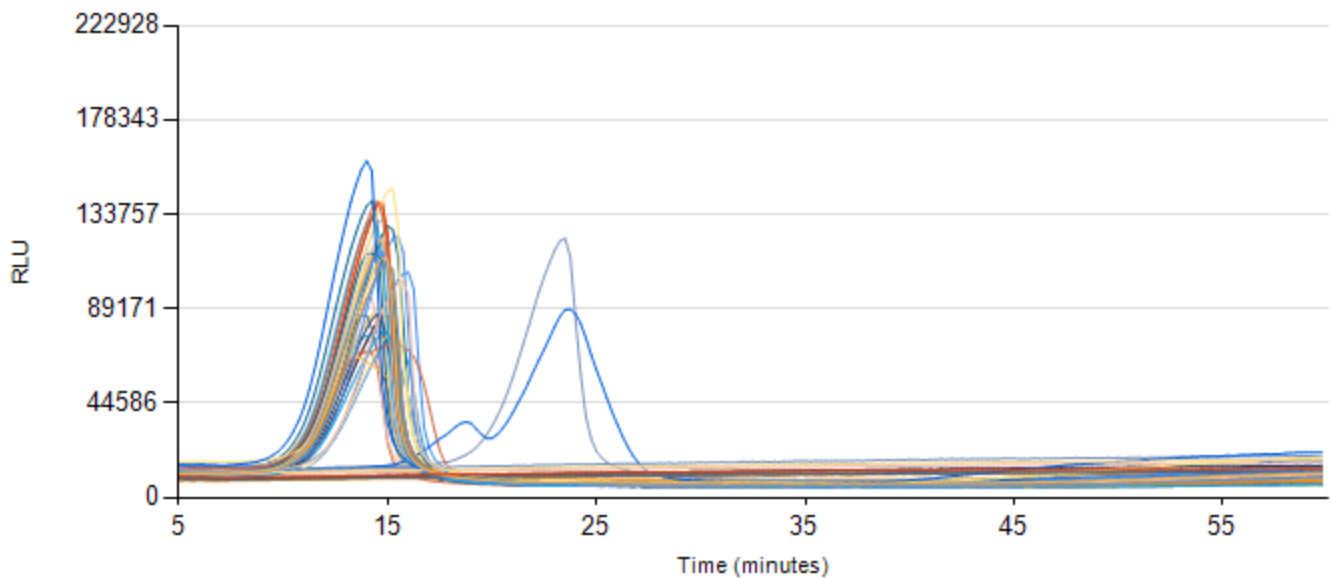

Molecular Detection Software

Run Report









Run ID	MPN - Example	Run Date	8/4/2024 11:10:15 AM
Run Status	Completed	User	Joseph Capobianco
Technician	Joseph Capobianco	Report By	Joseph Capobianco
Run Comment	MPN - Example	Instrument	0218040024:218040024

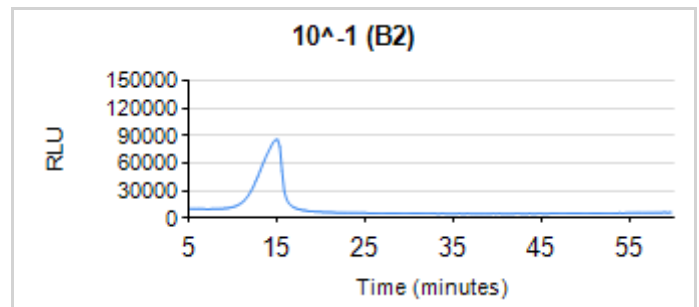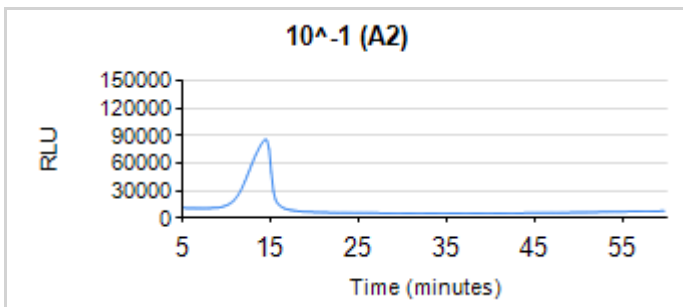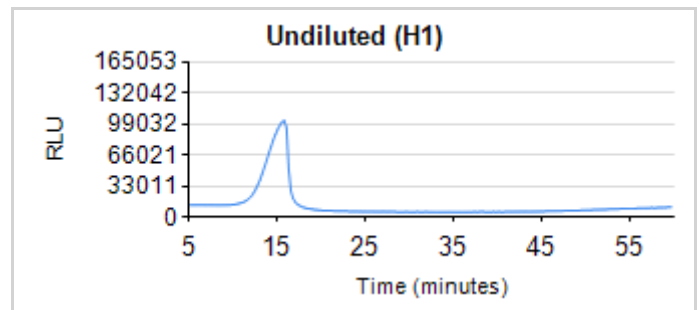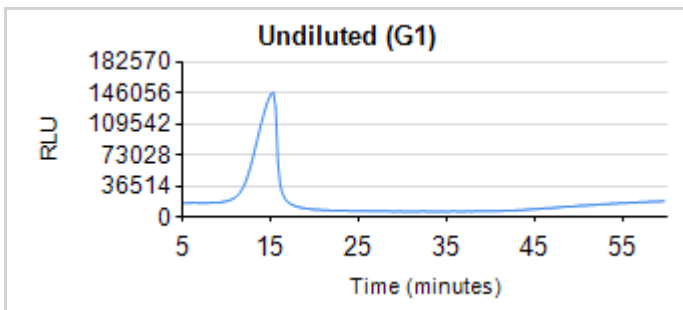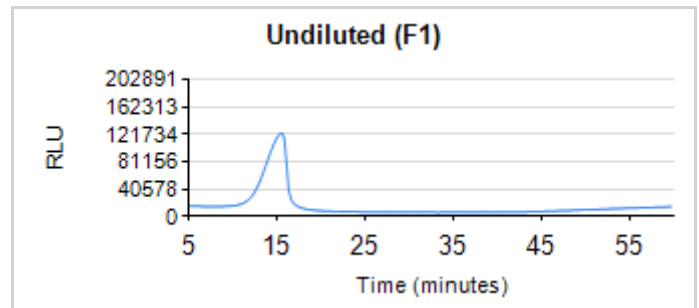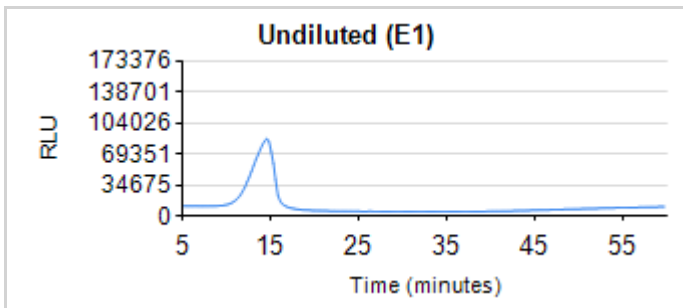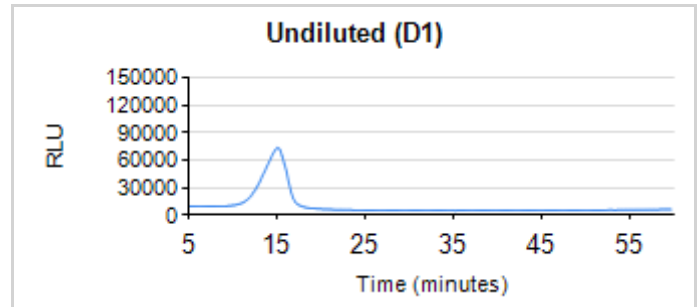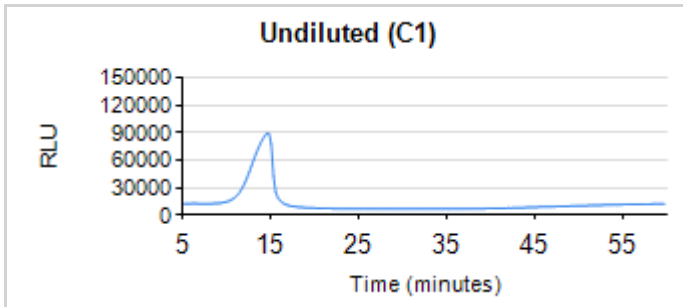

Molecular Detection Software

Run Report









Run ID	MPN - Example	Run Date	8/4/2024 11:10:15 AM
Run Status	Completed	User	Joseph Capobianco
Technician	Joseph Capobianco	Report By	Joseph Capobianco
Run Comment	MPN - Example	Instrument	0218040024:218040024

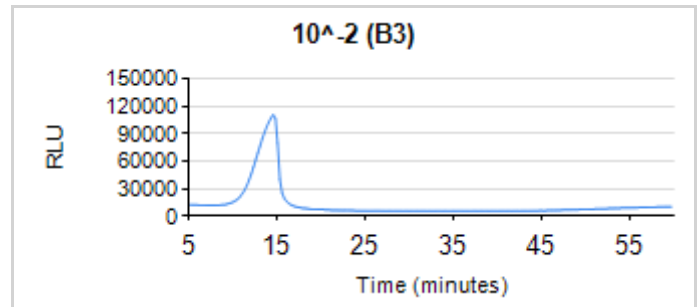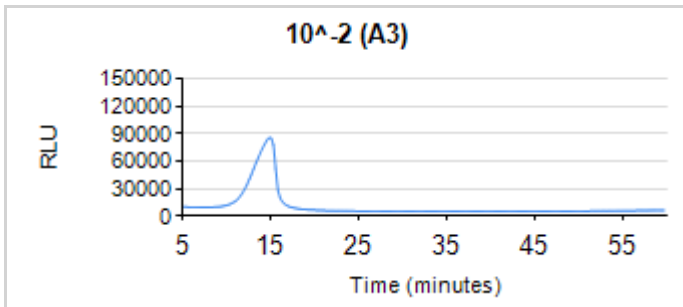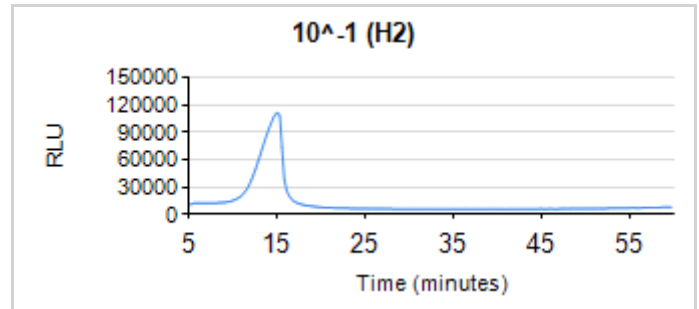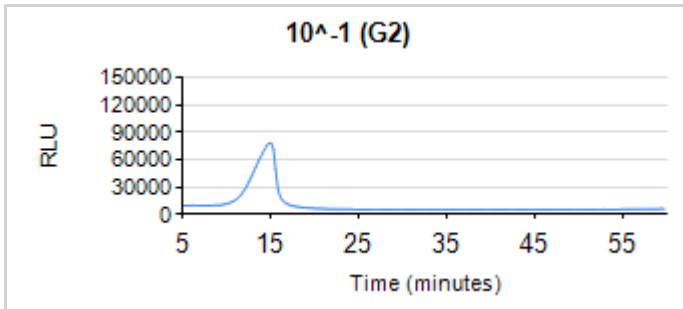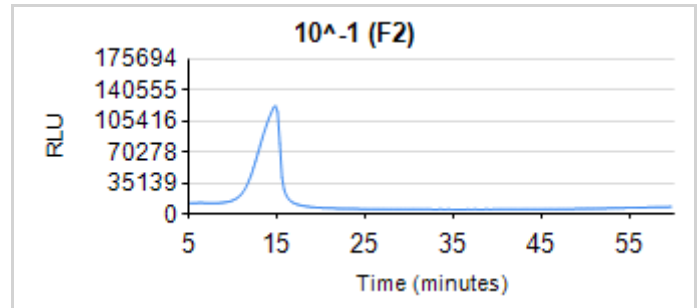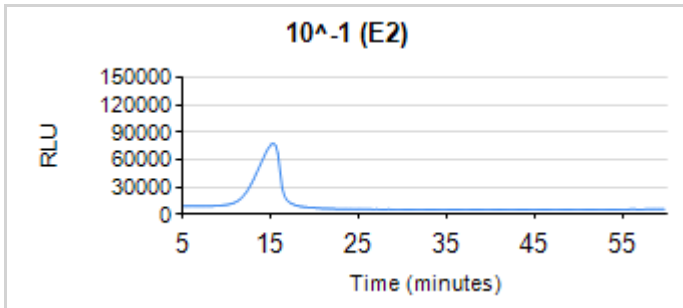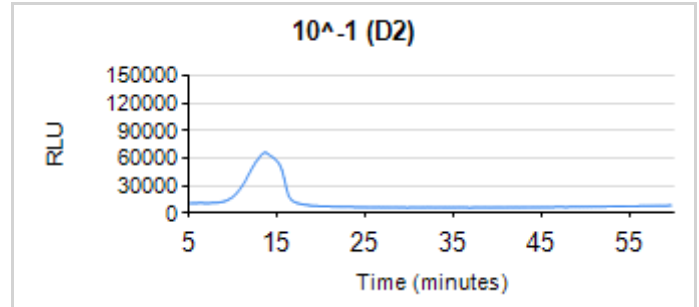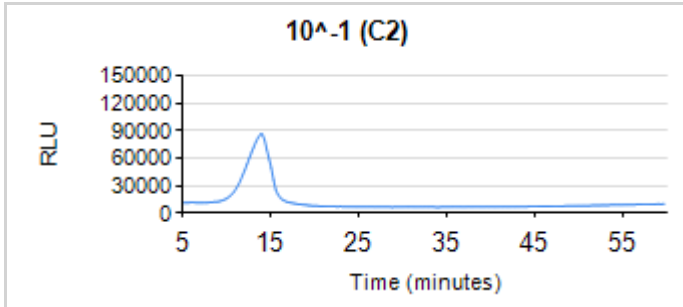

Molecular Detection Software

Run Report









Run ID	MPN - Example	Run Date	8/4/2024 11:10:15 AM
Run Status	Completed	User	Joseph Capobianco
Technician	Joseph Capobianco	Report By	Joseph Capobianco
Run Comment	MPN - Example	Instrument	0218040024:218040024

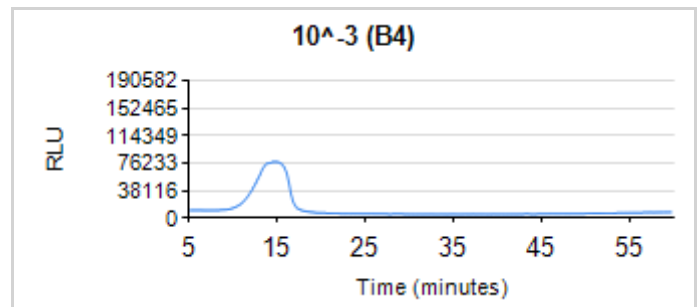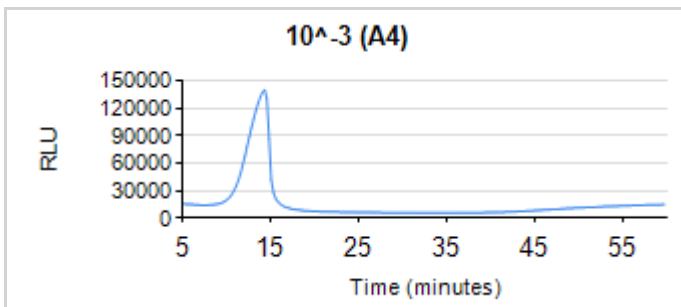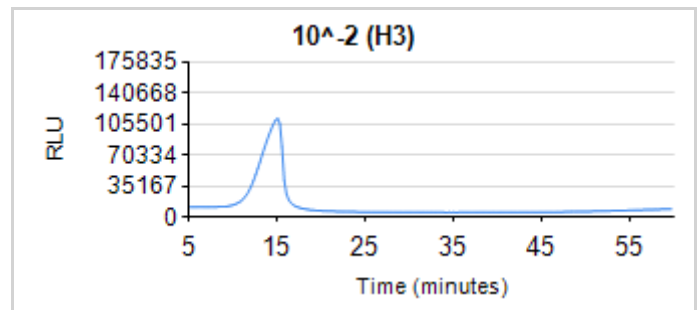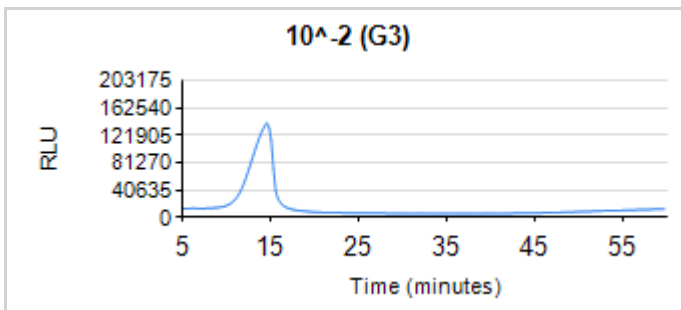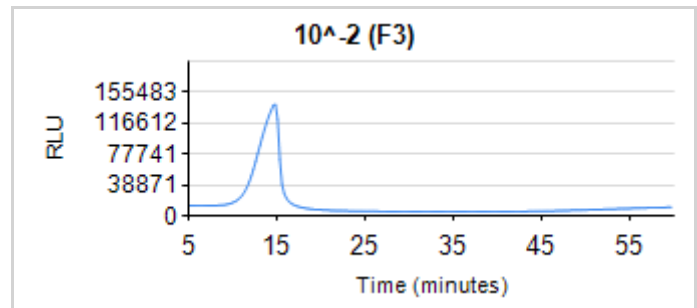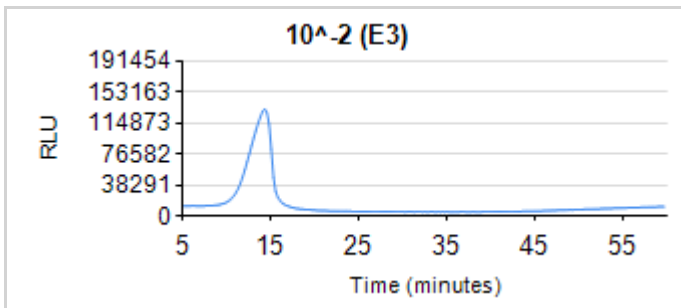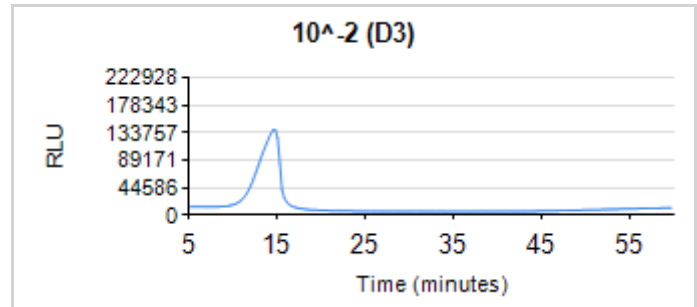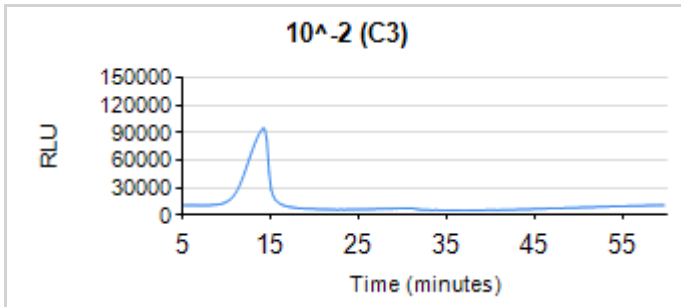

Molecular Detection Software

Run Report









Run ID	MPN - Example	Run Date	8/4/2024 11:10:15 AM
Run Status	Completed	User	Joseph Capobianco
Technician	Joseph Capobianco	Report By	Joseph Capobianco
Run Comment	MPN - Example	Instrument	0218040024:218040024

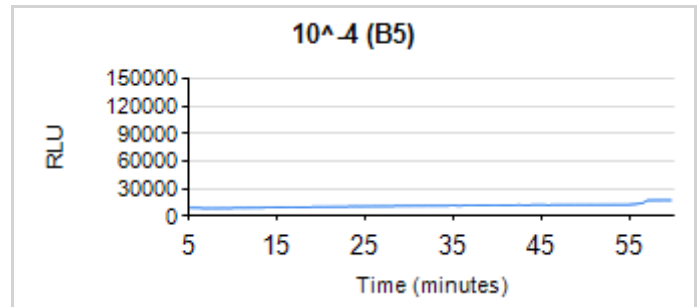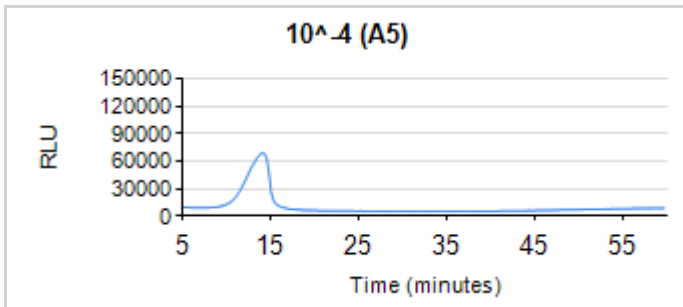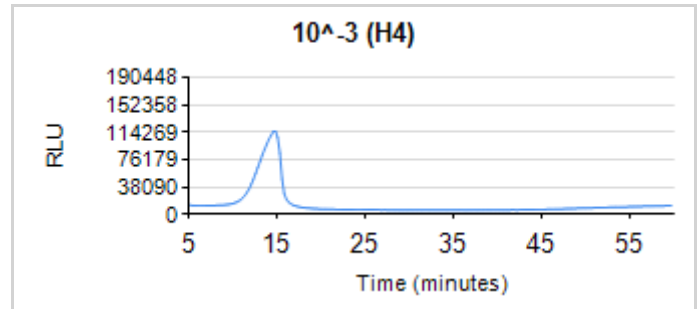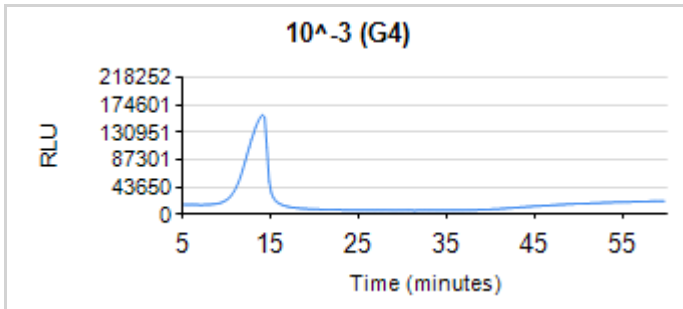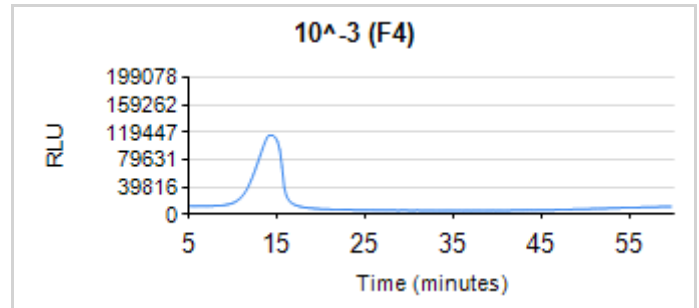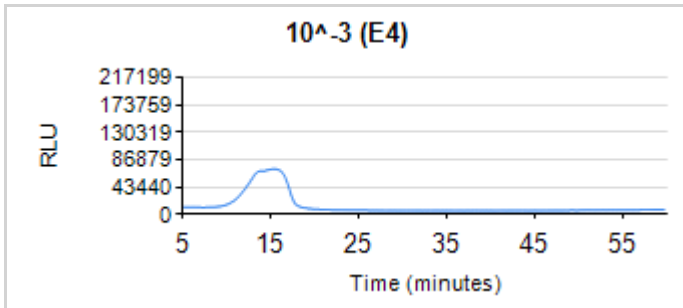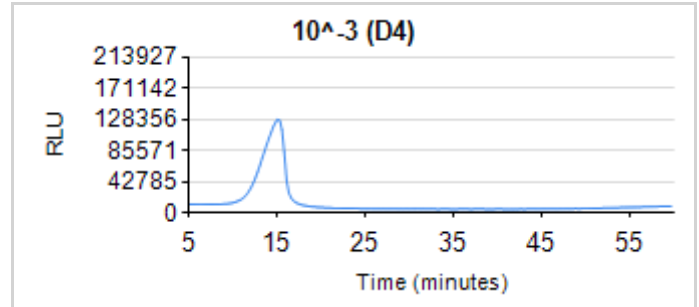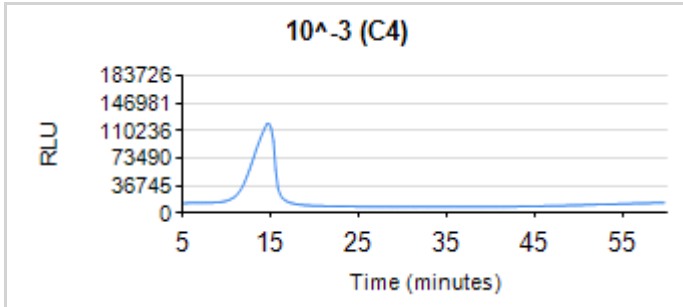

Molecular Detection Software

Run Report

Run ID	MPN - Example	Run Date	8/4/2024 11:10:15 AM
Run Status	Completed	User	Joseph Capobianco
Technician	Joseph Capobianco	Report By	Joseph Capobianco
Run Comment	MPN - Example	Instrument	0218040024:218040024

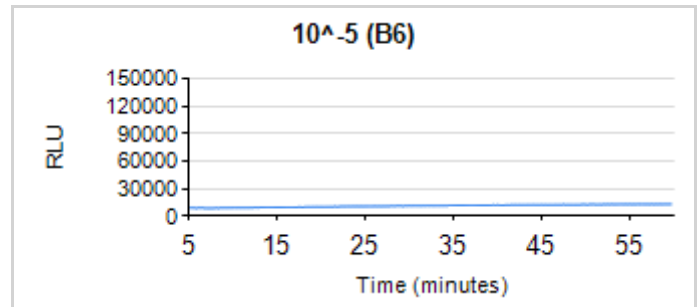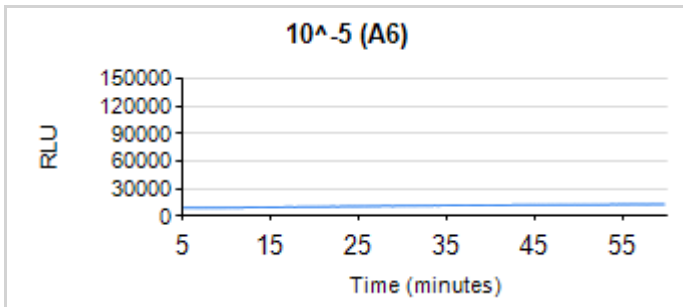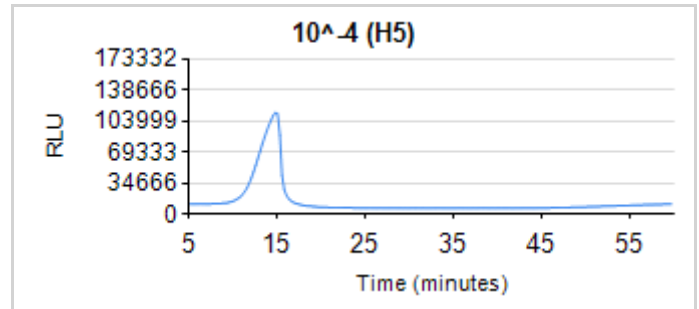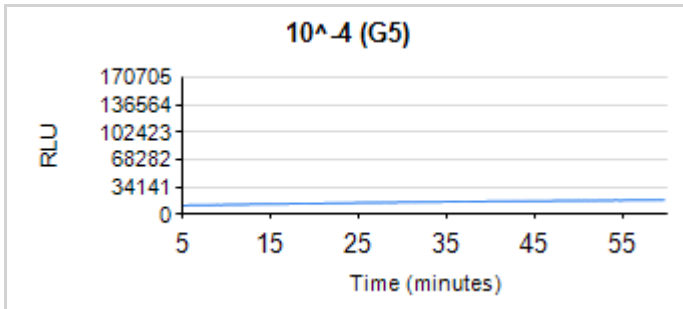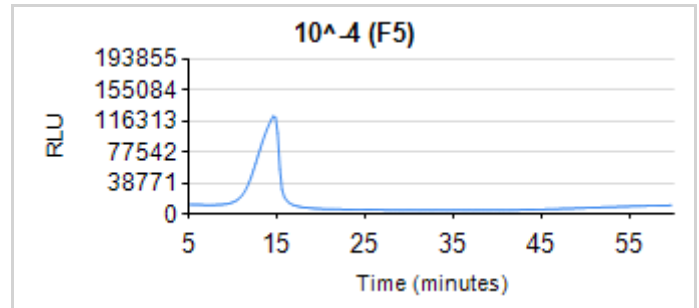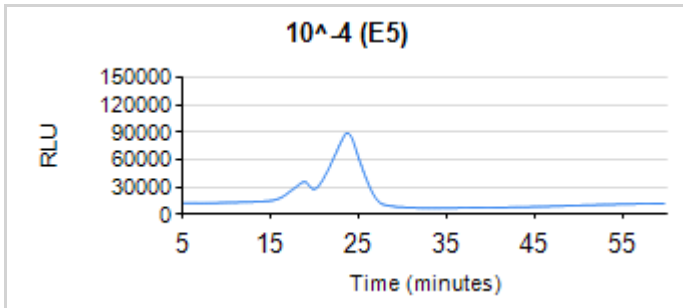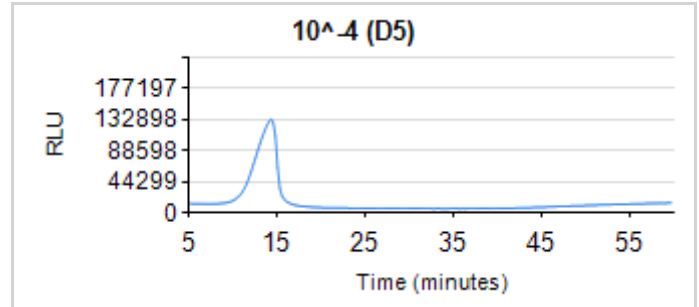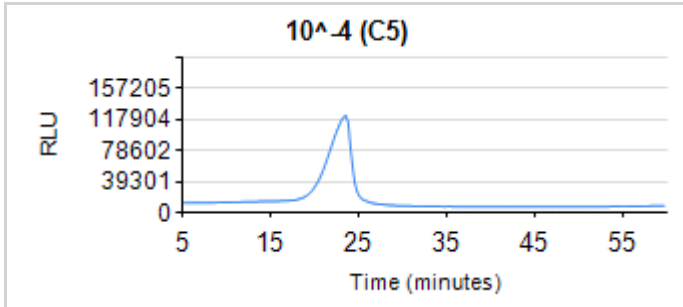

Molecular Detection Software

Run Report

Run ID	MPN - Example	Run Date	8/4/2024 11:10:15 AM
Run Status	Completed	User	Joseph Capobianco
Technician	Joseph Capobianco	Report By	Joseph Capobianco
Run Comment	MPN - Example	Instrument	0218040024:218040024

