

Video Article

# Colorimetric Paper-based Detection of *Escherichia coli*, *Salmonella* spp., and *Listeria monocytogenes* from Large Volumes of Agricultural Water

Bledar Bisha<sup>1</sup>, Jaclyn A. Adkins<sup>2</sup>, Jana C. Jokerst<sup>3</sup>, Jeffrey C. Chandler<sup>1</sup>, Alma Pérez-Méndez<sup>4</sup>, Shannon M. Coleman<sup>4</sup>, Adrian O. Sbodio<sup>5</sup>, Trevor V. Suslow<sup>5</sup>, Michelle D. Danyluk<sup>6</sup>, Charles S. Henry<sup>2</sup>, Lawrence D. Goodridge<sup>7</sup>

<sup>1</sup>Department of Animal Science, University of Wyoming

<sup>2</sup>Department of Chemistry, Colorado State University

<sup>3</sup>Department of Environmental and Radiological Health Sciences, Colorado State University

<sup>4</sup>Department of Animal Sciences, Colorado State University

<sup>5</sup>Department of Plant Sciences, University of California, Davis

<sup>6</sup>Department of Food Science and Human Nutrition, Citrus Research and Education Center, University of Florida

<sup>7</sup>Department of Food Science and Agricultural Chemistry, McGill University

Correspondence to: Bledar Bisha at [bbisha@uwyo.edu](mailto:bbisha@uwyo.edu)

URL: <https://www.jove.com/video/51414>

DOI: [doi:10.3791/51414](https://doi.org/10.3791/51414)

**Keywords:** Environmental Sciences, Issue 88, Paper-based analytical device (μPAD), Colorimetric enzymatic detection, *Salmonella* spp., *Listeria monocytogenes*, *Escherichia coli*, Modified Moore Swab (MMS), agricultural water, food safety, environmental microbiology

Date Published: 6/9/2014

**Citation:** Bisha, B., Adkins, J.A., Jokerst, J.C., Chandler, J.C., Pérez-Méndez, A., Coleman, S.M., Sbodio, A.O., Suslow, T.V., Danyluk, M.D., Henry, C.S., Goodridge, L.D. Colorimetric Paper-based Detection of *Escherichia coli*, *Salmonella* spp., and *Listeria monocytogenes* from Large Volumes of Agricultural Water. *J. Vis. Exp.* (88), e51414, doi:10.3791/51414 (2014).

## Abstract

This protocol describes rapid colorimetric detection of *Escherichia coli*, *Salmonella* spp., and *Listeria monocytogenes* from large volumes (10 L) of agricultural waters. Here, water is filtered through sterile Modified Moore Swabs (MMS), which consist of a simple gauze filter enclosed in a plastic cartridge, to concentrate bacteria. Following filtration, non-selective or selective enrichments for the target bacteria are performed in the MMS. For colorimetric detection of the target bacteria, the enrichments are then assayed using paper-based analytical devices (μPADs) embedded with bacteria-indicative substrates. Each substrate reacts with target-indicative bacterial enzymes, generating colored products that can be detected visually (qualitative detection) on the μPAD. Alternatively, digital images of the reacted μPADs can be generated with common scanning or photographic devices and analyzed using ImageJ software, allowing for more objective and standardized interpretation of results. Although the biochemical screening procedures are designed to identify the aforementioned bacterial pathogens, in some cases enzymes produced by background microbiota or the degradation of the colorimetric substrates may produce a false positive. Therefore, confirmation using a more discriminatory diagnostic is needed. Nonetheless, this bacterial concentration and detection platform is inexpensive, sensitive (0.1 CFU/ml detection limit), easy to perform, and rapid (concentration, enrichment, and detection are performed within approximately 24 hr), justifying its use as an initial screening method for the microbiological quality of agricultural water.

## Video Link

The video component of this article can be found at <https://www.jove.com/video/51414/>

## Introduction

It is important that foodborne disease agents are detected rapidly and preferably in field-based settings in order to reduce the burden of foodborne disease. Common strategies to detect foodborne bacterial pathogens include biochemical profiling, selective and differential culturing, immunological isolation and detection, and molecular detection. However, these methods are hampered by sporadic contamination, small sample sizes tested, the often low concentrations of the foodborne pathogenic bacteria, require long processing times, and/or are not applicable for field settings. Further, compounds in many food matrices are inhibitory to detection and diagnostic applications. In order to improve the likelihood of microbial detection, the United States Food and Drug Administration has suggested that testing agricultural water (such as wash water and irrigation water) which either comes in contact with a large surface area of fresh produce or serves as a vehicle for produce contamination is a viable alternative to direct testing of food<sup>1</sup>. Even so, the often low natural pathogen-burden coupled with the dilution effect of the representative agricultural water sample makes sample preparation methods for pathogen concentration essential. Such a method would require sampling large volumes of water (≥10 L), adequate pathogen-concentration, and compatibility with downstream detection strategies.

Modified Moore swabs (MMS) are inexpensive, simple, and rugged devices used for concentrating bacteria from large volumes (≥10 L) of water<sup>2-4</sup>. The MMS consists of a plastic cassette filled with gauze, which serves as a coarse filter for large volumes of water pumped through the cassette using a peristaltic pump. The MMS is a non-discriminatory method of bacterial concentration (≥10 fold concentration) that captures organic and inorganic particulate material including microorganisms in processed liquid samples. It is likely that the excellent efficacy of concentration of target microorganisms by the MMS can be explained by the fact that microorganisms are expected to be attached to the silt-

clay fraction or organic micro-aggregates of the suspended solids<sup>3</sup>. The rugged design of the MMS allows for overcoming most shortcomings associated with other filtration methods for capture and concentration of bacteria from water, such as clogging of filters, inability to process large volumes, filter samples with high turbidity, and high costs. For these reasons, the FDA is recommending that MMS's be incorporated into official procedures for environmental and produce-related sample collection procedures<sup>5</sup>.

Here, a method is described for the concentration, enrichment, and detection of *Escherichia coli*, *Salmonella* spp., and *Listeria monocytogenes* from agricultural waters. A MMS is used for concentration of bacteria, and also serves as a vessel for selective or non-selective bacterial enrichment. Bacterial detection is achieved biochemically using paper-based analytical devices ( $\mu$ PADs)<sup>6</sup>.  $\mu$ PADs can be manufactured as fluidic networks or spot tests using a variety of methods including photolithography, inkjet printing, stamping, and wax printing<sup>7-11</sup>. Examples of fluidic designs can be dendritic channel patterns where the sample is deposited in the center and subsequently flows to distal reservoirs or single channel patterns in which the sample or substrate are pulled from the outer reservoirs of the channel by capillary action into the center<sup>12</sup>. For this protocol, we have chosen to employ for 7-mm-diameter wax-paper spot arrays imbedded with chromogenic substrates that can be processed by enzymes indicative of the microorganisms tested here: Chlorophenol red  $\beta$ -D-galactopyranoside (CPRG) and 5-bromo-4-chloro-3-indolyl  $\beta$ -D-glucuronide (X-Gluc) for detection of  $\beta$ -galactosidase and  $\beta$ -glucuronidase produced by *E. coli*; 5-bromo-6-chloro-3-indolyl caprylate (magenta caprylate) for the detection of C8-esterase produced by *Salmonella* spp.; and 5-bromo-4-chloro-3-indolyl-myo-inositol phosphate (X-InP) for detection of phosphatidylinositol-specific phospholipase C (PI-PLC) produced by *L. monocytogenes*<sup>6</sup>. Thus, the presence of a particular bacterium can be observed visually without the need for complex equipment or data interpretation. The specificity and sensitivity of the enzyme-based colorimetric  $\mu$ PAD detection of these specific target bacteria has been previously explored<sup>6</sup>. In addition, the sensitivity of the integrated concentration-detection method for these target bacteria was evaluated by spiking of large volumes of water with pre-determined levels of microorganisms (unpublished data and Bisha *et al.*<sup>13</sup>).

## Protocol

### 1. Concentration of Bacteria from Large Volumes of Agricultural Water Using MMS

1. MMS Preparation
  1. Cut a rectangular section of 4-ply cheesecloth measuring 40 x 12 cm.
  2. Fold the cheesecloth along both axes to obtain a rectangle of 20 x 6 cm.
  3. Roll the cheesecloth tightly along its long axis to form a cylindrical swab of approximately 6 cm tall and 3 cm in diameter.
  4. Autoclave the cheesecloth swab in aluminum foil, do not autoclave the cassette. Decontaminate the cassette by soaking it for 30 min in 10% household bleach, and deactivate the residual chlorine by soaking the cassette for 15 min in a sodium thiosulfate pentahydrate ( $\text{Na}_2\text{S}_2\text{O}_3 \cdot 5\text{H}_2\text{O}$ ) solution (50 mg/L prepared in sterile water).
  5. Insert the swab into the MMS cassette.  
NOTE: If the non-disposable version of the MMS cassette is used, start with a 4-ply sheet of cheesecloth measuring 80 x 22 cm, fold it to 40 x 11 cm and roll it to form a cylinder approximately 11 cm tall and 6 cm in diameter.
  6. Assemble the MMS.
  7. Attach vinyl tubing to spigots on both sides of the MMS, ensuring the tubing fully adheres to the spigots, and fix tubing into the peristaltic pump. Ensure that the tubing upstream of the peristaltic pump is of sufficient length for sampling.
2. Concentration of Bacteria
  1. Sample at least 10 L of agricultural water by running the peristaltic pump at high speed.
  2. After sampling is complete, withdraw the peristaltic pump inlet from the water sample and continue running the pump until no effluent water is observed exiting the MMS.
  3. If a manifold is used to run several samples at the same time, collect the effluent of each MMS, and when 10 L is filtered through a single MMS close the valve for that particular MMS and continue running the pump.
    1. When sampling is completed, withdraw the peristaltic pump inlet from the agricultural water, open all the valves of the manifold, and continue running the pump until no effluent water is observed exiting the MMSs.
3. When concentration has been completed for all MMSs, carefully remove the vinyl tubing from the MMS spigots and cap the spigots on both sides of the MMS. Tightly capped MMS can be stored for up to 12 hr before adding enrichment media.

### 2. MMS Enrichment and Sample Preparation

1. Enrichment
  1. Unscrew the lid of the MMS, and aseptically add 20 ml of the appropriate sterile enrichment broth. Use one MMS for each selective enrichment. Alternatively, perform a non-selective enrichment to propagate all three target bacteria in the same sample.  
NOTE: If the non-disposable version of the MMS cassette is used, aseptically remove cheesecloth filter from the cassette and place in a sterile bag before adding 225 ml of the appropriate enrichment media.
    1. For enrichment of *E. coli*, add 20 ml of buffered peptone water (BPW) supplemented with 8 mg/L of vancomycin hydrochloride.
    2. For enrichment of *Salmonella* spp., add 20 ml of BPW supplemented with the *Salmonella* supplement (4 ml/L).
    3. For enrichment of *L. monocytogenes*, add 20 ml of VIDAS UP Listeria (LPT) broth.
    4. For simultaneous non-selective enrichment for all three microorganisms using a single MMS, use universal preenrichment broth (UPB).
  2. Screw the lid of the MMS back on tightly. Ensure that the spigots are tightly capped to avoid spills and possible contamination during enrichment.

3. Incubate the MMS for up to 18-24 hr in a shaking incubator at 200 rpm. Use 42 °C for *E. coli* and *Salmonella* spp. selective enrichments. Use 30 °C for *L. monocytogenes* selective enrichment, and use 37 °C for non-selective enrichment.
2. Sample Preparation
  1. When incubation has completed, remove the MMS from the incubator, uncap one of the spigots, and gently dispense about 0.5 ml into a 1.5 ml microcentrifuge tube. Alternatively, unscrew the MMS and pipette out 0.5 ml of overnight enrichment.  
NOTE: If the not-disposable version of the MMS cassette is used, pipette 0.5 ml of enrichment from the bag.
  2. For colorimetric analysis of *E. coli* selective enrichment, or for the analysis of the non-selective enrichments, sonicate 0.5 ml of enrichment at 5 W, 22 kHz for 20 sec using a probe sonicator.

### 3. Preparation and Embedding of Colorimetric Substrates in $\mu$ PADs

1. Prepare enough  $\mu$ PADs for each sample and target tested. To detect *E. coli* prepare CPRG and X-Gluc  $\mu$ PADs, for *Salmonella* spp. detection prepare MC  $\mu$ PADs, and for *L. monocytogenes* detection prepare X-InP  $\mu$ PADs.
  1. Prepare HEPES buffer [0.1 M HEPES with 0.1% Bovine Serum Albumin (BSA)] for the colorimetric substrates and adjust the pH of the buffer according to the substrate that is going to be used: pH 7.5 for preparation of CPRG or X-Gluc, pH 9 for MC, and pH 7 for X-InP.
  2. Prepare stock solutions of the substrates in the pH adjusted HEPES buffer at concentrations of 3 mM (CPRG), 62.5 mM (X-Gluc), 15 mM (MC), 100 mM (X-InP). Protect the stock solutions from light.
  3. Place the  $\mu$ PADs inside a sterile Petri dish, then imbed the  $\mu$ PAD microspot with 24  $\mu$ l of each substrate stock solution.


### 4. Detection and Data Analysis

1. Detection
  1. Add 6  $\mu$ l of the enriched sample to each appropriate  $\mu$ PAD microspot contained in a Petri dish.
  2. Place the cover back on the Petri dish and seal it with Parafilm.
  3. Incubate the sample with the  $\mu$ PAD at 37 °C for up to 3 hr to allow for color development and drying of the microspots.
2. Visual Examination of the Results
  1. Perform detection by simple visual inspection of the color changes of the  $\mu$ PADs.  
NOTE: Typically, strong reactions that produce definitive color changes are expected following 18-24 hr of enrichment, which should obviate the need for further clarification and should be considered positive.
  2. Determine the presence of an *E. coli* positive sample by observing microspots imbedded with CPRG change from yellow to red-violet and microspots imbedded with X-Gluc change from colorless to blue-green.
  3. Determine the presence of a *L. monocytogenes* positive sample by observing microspots imbedded with X-InP change from colorless to indigo.
  4. Determine the presence of a *Salmonella* spp. positive sample by observing microspots imbedded with MC change from colorless to purple-mauve.
3. Software Aided Data Analysis  
NOTE: Conducted to clearly determine whether weak reactions are positive or negative and to enable a semi-quantitative analysis of the results.
  1. Allow the  $\mu$ PADs to fully dry.
  2. Scan the  $\mu$ PAD using a flat-bed scanner.
  3. Use ImageJ software to process the image.
    1. "Open" scanned image to be analyzed in ImageJ located under the "File" tab on the main menu (or press "Clt+O").
    2. Invert the image selecting "Invert" located under the "Edit" tab on the main menu (or press "Clt+Shift+I").
    3. Use the "Analyze" tab on the main menu and select "Set Measurements..." to select the reported measurements analyzed.
    4. Make sure that the "Mean grey intensity," "Limit to threshold," and "Display label" boxes are checked, and press "OK." This sets how the software analyzes each area selected and how it reports it.
    5. Use the "Oval" tool to draw a circle that outlines the area that you want to measure within.
    6. Under the "Analyze" tab select "Measure," (or press "Clt+M"). The software will measure the average grey intensity within the area defined and report it in a pop-up screen that can be copied and pasted to excel for further analysis.  
NOTE: For more accurate analyses, at least two technical replicates of each sample should be performed.


## Representative Results

As described in this protocol, concentration of bacteria using the MMS (**Figure 1**) can be performed within approximately 15-20 min. The MMS is constructed from acrylonitrile butadiene styrene (ABS) in two separate components; a lid and a cartridge both with an integrated spigot assembly into which a cylindrical cheesecloth swab is inserted (**Figure 1A**). Both components are then screwed together forming the MMS (**Figure 1B**). MMS-based processing is driven by a battery-powered peristaltic pump, allowing for samples to be concentrated in field settings. By coupling MMS concentration, selective enrichments (18-24 hr), and  $\mu$ PADs; agricultural water can be rapidly (approximately 24 hr), easily, and cheaply screened for important foodborne pathogens and indicator microorganisms, including *E. coli*, *Salmonella* spp., and *L. monocytogenes*. With this protocol, these target bacteria can be detected at levels as low as 0.1 CFU/ml. The  $\mu$ PAD assays are based on the detection of bacteria-indicative enzymes that react with colorimetric substrates (**Figure 2**). Assays detecting *E. coli*, but not *E. coli* O157:H7, produce a blue-green product (**Figure 2A**). Similarly, the assay that detects a majority of *E. coli* strains produces a red-violet reaction product (**Figure 2B**). Assays


detecting *Salmonella* spp. (**Figure 2C**) and *L. monocytogenes* (**Figure 2D**) produce purple-mauve and indigo colors, respectively. The test can be interpreted by eye (qualitatively), and visual judgments are usually satisfactory for discriminating between positive and negative samples. Alternatively, digitized images can be manipulated using ImageJ software (**Figure 3A**) to allow for more objective and standardized data interpretation (**Figure 3B**).

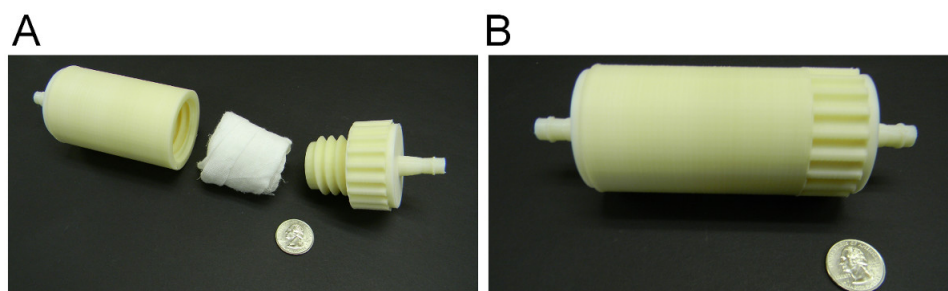

**Figure 1. The Modified Moore Swab (MMS) cassette.** (A) The disassembled MMS. The MMS is produced in a 3-D printer from acrylonitrile butadiene styrene (ABS) and consists of three main components: A cartridge with an incorporated spigot assembly into which a cylindrical cheesecloth swab (folded 4-ply) is inserted and is capped with a lid having an integrated spigot assembly. (B) The assembled MMS.

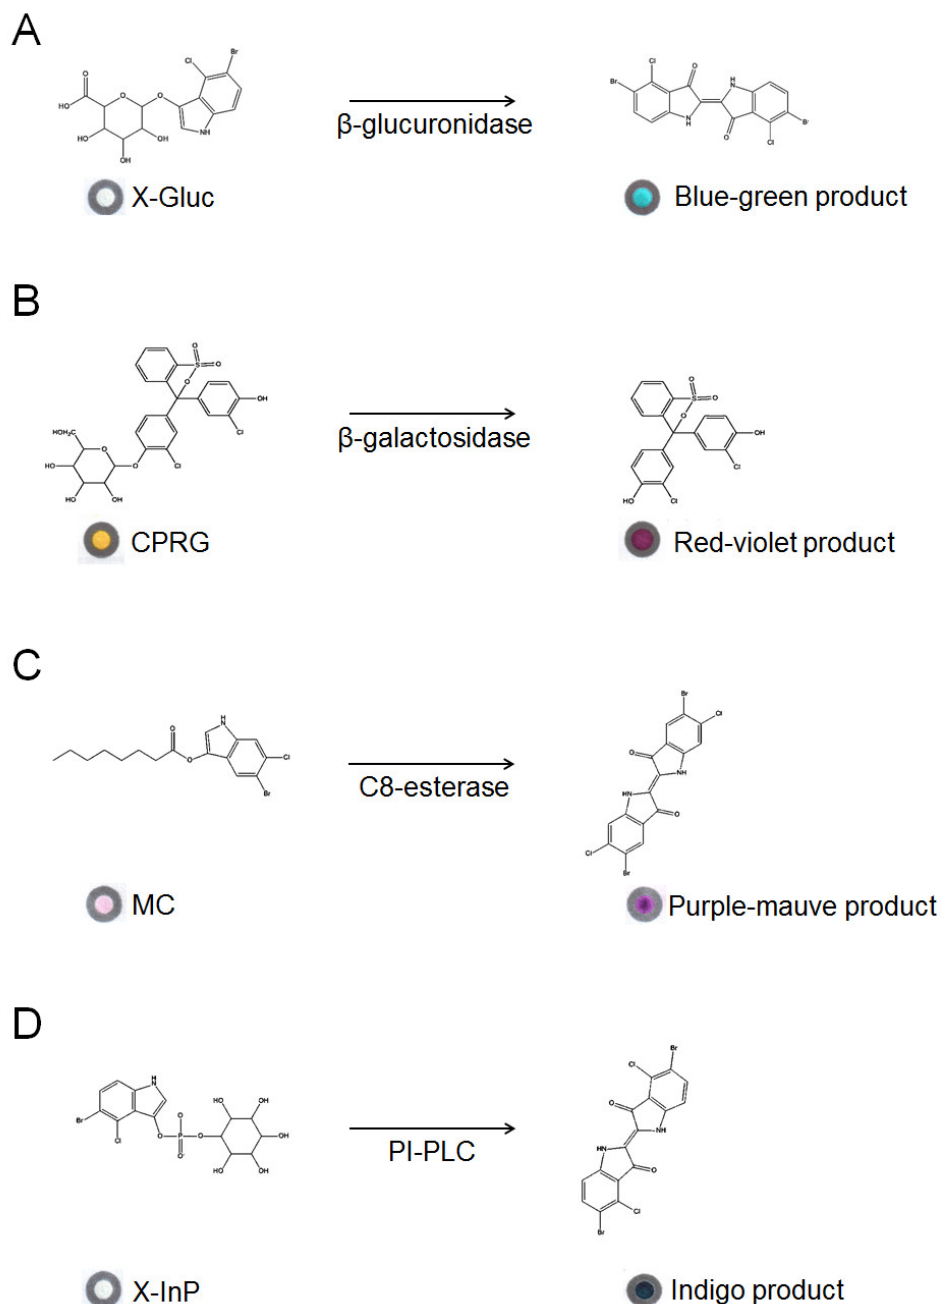

**Figure 2. Bacteria-indicative colorimetric reactions.** Substrates (X-Gluc, CPRG, MC, and X-InP) imbedded in the microspots of the  $\mu$ PADs react with bacteria-indicative enzymes ( $\beta$ -glucuronidase,  $\beta$ -galactosidase, C8-esterase, and PI-PLC) to produce a colorimetric change. **(A)** A positive X-Gluc reaction is an indication of generic *E. coli*, but not *E. coli* O157:H7; **(B)** a positive CPRG reaction is an indication that *E. coli* are present; **(C)** a positive MC reaction indicates the presence of *Salmonella* spp.; **(D)** and a positive X-InP reaction indicates the presence of *L. monocytogenes*.

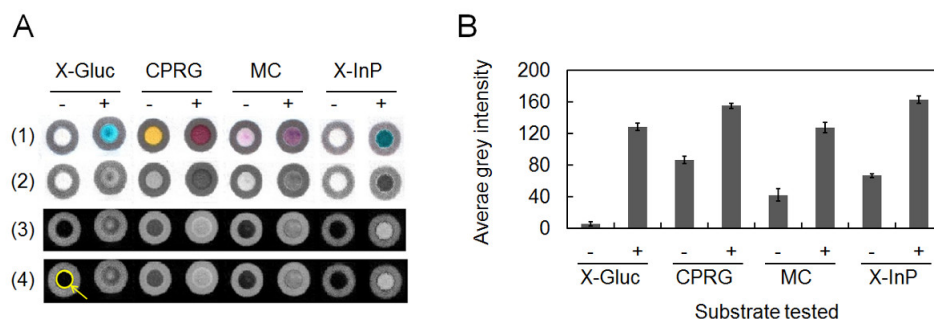

**Figure 3. Visual and ImageJ analyses of the bacteria-indicative colorimetric  $\mu$ PAD tests.** **A** shows digitized colorimetric images for each assay with both a negative (-) and positive (+) test. Negative tests were performed using lysates of bacterial species that do not encode the target enzymes and positive tests with lysates or enrichments of the target bacteria. (1) Unmodified scanned images. (2) Scanned images converted to greyscale using ImageJ software, and (3) color inverted images for subsequent interpretation of grey intensity. (4) Average grey intensity measured using ImageJ within each microspot of the  $\mu$ PAD (an example microspot is indicated by the yellow arrow and circle). **B** shows the average grey intensities (determined by ImageJ) for each colorimetric  $\mu$ PAD positive and negative test. [Please click here to view a larger version of this figure.](#)

## Discussion

This protocol describes an integrated method for detecting *E. coli*, *Salmonella* spp., and *L. monocytogenes* in agricultural water. Here, MMS concentration of bacteria from large volumes (10 L) of agricultural water, is coupled with bacterial enrichment, and bacterial-indicative colorimetric detection using  $\mu$ PADs. The MMS procedure can cope with high particulate content in the water samples while concentrating the bacteria 10-fold, is robust and simple enough for field applications by minimally trained personnel, and can be performed with minimal costs. By incorporating a bacterial enrichment step, live bacteria are detected and the sensitivity of the method is greatly enhanced. Enrichment amplifies the target to be assayed, and when combined with selective growth media, reduces unwanted microbiota growth in samples that could contribute to false positive results. Final detection is performed with  $\mu$ PADs, which provide a simple, cost effective, and easy to interpret solution to screen for important foodborne pathogens. The entire procedure, including MMS concentration, overnight enrichment, and colorimetric detection, can be performed within one day, and detects bacterial contamination at levels as few as 0.1 CFU/ml.

To simplify the method and reduce the possibility of contamination, the MMS is used as a container for bacterial enrichment. Adding this enrichment to the procedure increases sensitivity, specificity, adds flexibility into the method. Although only three selective enrichments were utilized here, improved enrichments for the bacteria could be developed. For example, we are exploring the possibility of incorporating specific inducers into the enrichment media to enhance the production of the reporter enzymes used for colorimetric detection.

The  $\mu$ PADs used for pathogen detection are simple-to-use single spot arrays that cost as little as \$0.002/device prior to the addition of the colorimetric reporter substrate. Even accounting for enrichment reagents and colorimetric substrates, the cost of each test is a few cents, except for the *L. monocytogenes* test which is estimated at \$1.28/test due to the currently high cost of X-InP. Nonetheless, this cost compares favorably to current detection methods for foodborne pathogens<sup>6</sup>. In their current form, the  $\mu$ PADs must be prepared immediately prior to testing due to poor substrate stability. To overcome this limitation, we are testing the addition of stabilizing additives and evaluating dry storage to increase substrate/ $\mu$ PAD shelf life. Additionally, we are developing multiplexed  $\mu$ PADs using several sample/reagent sites connected to each other by microfluidic channels.

Despite the advantages previously detailed for the  $\mu$ PAD testing, problems with assay specificity are possible: 1) The reporter enzymes are not exclusively produced by the target bacteria, thus contaminating background microbiota may contribute to a false positive result. 2) If dark colored particulate persists in the enrichment media, it can obscure visual and ImageJ analysis when transferred to the  $\mu$ PAD. 3) The current assay cannot specifically detect *E. coli* O157:H7. Consequently, the method is more suited as an initial screening test providing impetus for further testing and confirmation to be conducted. Nevertheless, many of these shortcomings are easily addressed. Incorporating a larger panel of indicative colorimetric substrates would allow for more precise determination of the target bacterium, including *E. coli* O157:H7. Similarly, additional selective enrichment procedures could minimize the contaminating microbiota in the sample. To reduce the impact of particulate in enrichments, a coarse filter could be used prior to applying samples to the  $\mu$ PAD.

In conclusion, this study demonstrates that the MMS combined with enrichment and  $\mu$ PADs can be used to detect low levels of *E. coli*, *Salmonella* spp. and *L. monocytogenes* in agricultural water. With few modifications, the procedure is portable and able to be applied in field settings.

## Disclosures

The authors have nothing to disclose.

## Acknowledgements

We gratefully acknowledge funding for this project from the USDA National Institute of Food and Agriculture grants 2009-01208 and 2009-01984.



## References

1. *Guidance for industry: Guide to minimize microbial food safety hazards for fresh fruits and vegetables*. U.S. Dept. of Health and Human Service, Food and Drug Administration, Center for Food Safety and Applied Nutrition (CFSAN), (1998).
2. Bisha, B., Pérez-Méndez, A., Danyluk, M. D., & Goodridge, L. D. Evaluation of Modified Moore swabs and continuous flow centrifugation for concentration of *Salmonella* and *Escherichia coli* O157:H7 from large volumes of water. *J Food Prot.* **74**, 1934-1937, doi:10.4315/0362-028X.JFP-11-133 (2011).
3. Sbodio, A., Maeda, S., Lopez-Velasco, G., & Suslow, T. V. Modified Moore swab optimization and validation in capturing *E. coli* O157:H7 and *Salmonella enterica* in large volume field samples of irrigation water. *Food Res Int.* **51**, 654-662, doi:DOI 10.1016/j.foodres.2013.01.011 (2013).
4. McEgan, R. *et al.* Detection of *Salmonella* spp. from large volumes of water by modified Moore swabs and tangential flow filtration. *Lett Appl Microbiol.* **56**, 88-94, doi:10.1111/lam.12016 (2013).
5. Administration, U. S. F. a. D. in *Solicitation Number: FDA-SS-1116253*. (2013).
6. Jokerst, J. C. *et al.* Development of a paper-based analytical device for colorimetric detection of select foodborne pathogens. *Analytical Chemistry*. **84**, 2900-2907, doi:Doi 10.1021/Ac203466y (2012).
7. Martinez, A. W., Phillips, S. T., Butte, M. J., & Whitesides, G. M. Patterned paper as a platform for inexpensive, low-volume, portable bioassays. *Angew Chem Int Edit.* **46**, 1318-1320, doi:DOI 10.1002/anie.200603817 (2007).
8. Martinez, A. W., Phillips, S. T., Wiley, B. J., Gupta, M., & Whitesides, G. M. FLASH: A rapid method for prototyping paper-based microfluidic devices. *Lab on a Chip.* **8**, 2146-2150, doi:Doi 10.1039/B811135a (2008).
9. Abe, K., Suzuki, K., & Citterio, D. Inkjet-printed microfluidic multianalyte chemical sensing paper. *Analytical Chemistry*. **80**, 6928-6934, doi:Doi 10.1021/Ac800604v (2008).
10. Cheng, C. M. *et al.* Millimeter-scale contact printing of aqueous solutions using a stamp made out of paper and tape. *Lab on a Chip.* **10**, 3201-3205, doi:Doi 10.1039/C004903d (2010).
11. Lu, Y., Shi, W. W., Jiang, L., Qin, J. H., & Lin, B. C. Rapid prototyping of paper-based microfluidics with wax for low-cost, portable bioassay. *Electrophoresis*. **30**, 1497-1500, doi:DOI 10.1002/elps.200800563 (2009).
12. Charles, S., Henry, L. D. G., Jana, C. Jokerst. *Rapid detection of pathogens using paper devices*. United States patent WO2012125781 A3 (2012).
13. Bisha, B., *et al.* T10-06 Colorimetric paper-based detection of *Salmonella* spp. and *Escherichia coli* from artificially contaminated irrigation river water. *International Association for Food Protection Annual Meeting*. Providence, RI. (2012).